

Quality is more than a word

ESPEC

Elevator type

Thermal Shock Chamber

TSD-101-W

TSE-12-A



Two-zone chamber capable of exposing specimens to a uniform thermal stress.

These two-zone thermal shock chambers are designed to specifically meet the needs of MIL, IEC, JASO and other international testing standards.

Choose from small, medium, from 10L to 300L to fit your testing.

They come mounted with The N-instrumentation for improved operability and visibility, making remote monitoring and control via an Ethernet connection possible from your desk. Thermal shock chambers that apply uniform levels of thermal stress to specimens and that can be used in a wide range of fields, from research and development through to inspections and production.

11L



TSE-12-A

70L



TSD-71-A

To minimize our chambers potential environmental impact

R-449A is the best alternative to R-404A



*R-449A is available on request

100L



TSD-101-W

300L



TSD-301-W

*The viewing window, casters (TSD) and recorder, emergency stop pushbutton (TSE) are optional.

Features

Reduce test time with a two-zone elevator type

Line-up

Model		Volume	Test area
TSE-12-A	Air-cooled	10.9L	W320×H148×D230mm
TSD-71-A		70L	W560×H345×D370mm
TSD-101-W	Water-cooled	100L	W710×H345×D410mm
TSD-301-W		275L	W650×H650×D650mm


● TSD specimen temperature recovery example (based on MIL-STD-883 Method 1010.9)

Test conditions

Hot exposure: +150°C for 30 min.
Cold exposure: -65°C for 30 min.
Specimens: ICs, 10 kg

Measurement conditions

Thermocouples were embedded in 10 ICs placed on two levels in each corner and in the center of a specimen basket.
(Specimens embedded with thermocouples were placed beneath other ICs.)

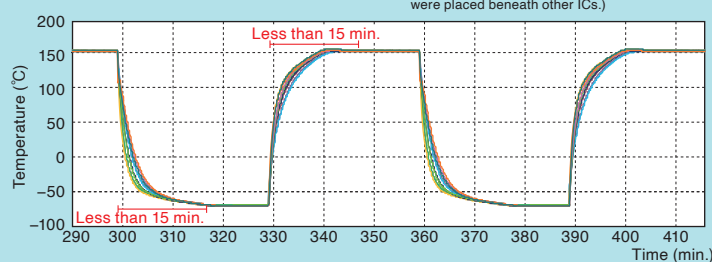


● TSD temperature uniformity example

Test conditions

Hot exposure: +150°C for 30 min.
Cold exposure: -65°C for 30 min.
Specimens: ICs (×10)

Measurement conditions

Thermocouples were attached to the surface of 10 ICs placed on two levels in each corner and in the center of a specimen basket.

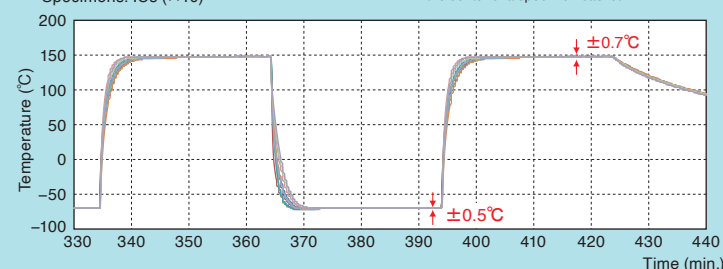

● Short temperature recovery time

● Meets international standards

Designed to comply with major environmental test standards such as IEC, JEDEC, EIAJ, MIL, JASO, IPC and SAE. (p.5 ~ 6)

● Transfer time within 10sec.

Test area transfer time between hot/cold chamber meets international test standards requirement.
(TSD-101-W, TSE-12-A)

● Improved temperature uniformity

Uniform airflow in the test area allows outstanding temperature uniformity. Uniform thermal stress is applied to each specimen, minimizing variation in test results.

● Smooth specimen transfer

“Soft move mode” is automatically activated when specimens move between the hot and cold chambers to reduce vibration and shock.



TSD



TSE



TSE hot exposure



TSE cold exposure

● Test area anti-drop mechanism to protect specimens

The test area's drive unit is equipped with a braking device to prevent specimens from falling the test area under any abnormal situations. For testing of small test samples, the specimen protective mesh which covered entire test area can be added. (Option)

Features

● Easy wiring access

A cable port on right side allows for easy wiring for specimen measurement.



● Specimen Temperature Trigger (STT)

With up to two sensors attached to specimen(s), the STT function begins counting the exposure time once the specimen reaches a set temperature, or promptly activates moving of the specimen for the next exposure. This reduces overall testing time and ensures accurate specimen temperatures. Temperature readings can be recorded for each specimen and test area by connecting a temperature recorder. (TSD)



● Safe specimen handling thanks to ambient temperature recovery

The ambient temperature recovery feature intakes external air to return the test area to an ambient temperature after testing has finished or been paused. (TSD)

● Comprehensive safety system

A double safety system ensures that any transfer between test areas stops automatically when the door is open, and that the door locks while transfer is in progress.



TSD-101-W Specimen temperature measurement
(Specimen temperature sensors Standard: 2 sensors
Optional: additional 3 sensors)



TSD-101-W Test areas (Top: hot chamber
Bottom: cold chamber)

TEST STANDARD AND COMPATIBLE MODELS

Test standard		Temperature setting		Soak time	Recovery time	Number of cycles	Model *
		Hot (°C)	Cold (°C)				
IEC 60068-2-14 (JIS C 60068-2-14 DIN EN 60068-2-14 BS EN 60068-2-14)		+ 70 ± 2 + 85 ± 2 + 100 ± 2 + 125 ± 2 + 155 ± 2 + 175 ± 2 + 200 ± 2	− 5 ± 3 − 10 ± 3 − 25 ± 3 − 40 ± 3 − 55 ± 3 − 65 ± 3	3 hours 2 hours 1 hour 30 min. 10 min. 3 hours if not specified in product specifications	10% of soak time	5	TSD TSE
IEC 60749-25 (JESD22-A104F)	A	+ 85 (+ 10, − 0)	− 55 (+ 0, − 10)	1/ 5/ 10/ 15 min.	Specimen 5 to 14 min.	Not specified	TSD
	B	+ 125 (+ 15, − 0)	− 55 (+ 0, − 10)		Specimen 5 to 14 min.		
	C	+ 150 (+ 15, − 0)	− 65 (+ 0, − 10)		Specimen 5 to 29 min.		
	H	+ 150 (+ 15, − 0)	− 55 (+ 0, − 10)		Specimen 5 to 14 min.		
	M	+ 150 (+ 15, − 0)	− 40 (+ 0, − 10)		Specimen 5 to 15 min.		
IEC 61747-5 Na (EIAJ ED-2531A Na)		+ 100 ± 2 + 95 ± 2 + 90 ± 2 + 85 ± 2 + 80 ± 2 + 75 ± 2 + 70 ± 2 + 65 ± 2 + 60 ± 2	− 50 ± 3 − 45 ± 3 − 40 ± 3 − 35 ± 3 − 30 ± 3 − 25 ± 3 − 20 ± 3 − 15 ± 3 − 10 ± 3 − 5 ± 3 − 0 ± 3	3 hours 2 hours 1 hour 30 min. 10 min. 3 hours if not specified in product specifications	10% of soak time	5-10	TSD TSE
EIAJ ED-4701		Max. storage temp.	Min. storage temp.	15g and below: at least 10 min. 15 to 150g: at least 30 min. 150 to 1,500g: at least 60 min. More than 1,500g: individually specified	Air 5 min. or 10% of soak time, whichever is longer	10	TSD
EIAJ ED-4702	A	+ 125 (± 3)	− 65 (± 3)	30 min.	Air 5 min. or 10% of soak time, whichever is longer	5 cycles unless otherwise specified	TSD
	B	+ 100 (± 3)	− 65 (± 3)				
	C	+ 100 (± 3)	− 55 (± 3)				
	D	Mounted printed circuit board max. operating temp.	Mounted printed circuit board min. operating temp.				
EIAJ ET-7407	A	+ 125 ± 5	− 25 ± 5	7 min. after specimen temperature attainment	—	—	TSD
	B	+ 125 ± 5	− 40 ± 5				
	C	+ 80 ± 5	− 30 ± 5				
	D	Max. operating temp.	Min. operating temp.				


TEST STANDARD AND COMPATIBLE MODELS

Test standard		Temperature setting		Soak time	Recovery time	Number of cycles	Model *
		Hot (°C)	Cold (°C)				
MIL-STD-883 Method 1010.9	A	+ 85(+ 10, − 0)	− 55(+ 0, − 10)	10 min. or longer after transition start	Specimen less than 15 min.	At least 10	TSD TSE
	B	+ 125(+ 15, − 0)	− 55(+ 0, − 10)				
	C	+ 150(+ 15, − 0)	− 65(+ 0, − 10)				
	D	+ 200(+ 15, − 0)	− 65(+ 0, − 10)				
	F	+ 175(+ 10, − 0)	− 65(+ 0, − 10)				
JASO-D902	Type 1	+ 85	− 40	Within 5 min. after solder joint temp. reaches ±2°C of preset temp. Or, 0.2kg and below: 0.5 hours 0.2 to 0.8kg: 1 hour 0.8 to 1.5kg: 1.5 hours More than 1.5kg: 2 hours preset temp.	Air 5 min.	200	TSD
	Type 2	Depends on parties involved					
IPC-TM-650 2.6.6	A	+ 125(+ 3, − 0)	− 65(+ 0, − 5)	30 min.	————	5	TSD
	B	+ 85(+ 3, − 0)	− 55(+ 0, − 5)				
SAE J1879		+ 150	− 55	10 min. or longer after transition start	Specimen less than 15 min.	1000	TSD

* The test results may not meet specifications depending on the quantity of specimens or the setting method.

■ For further information, please contact us.

An easy-to-use, easy-to-read touch panel.

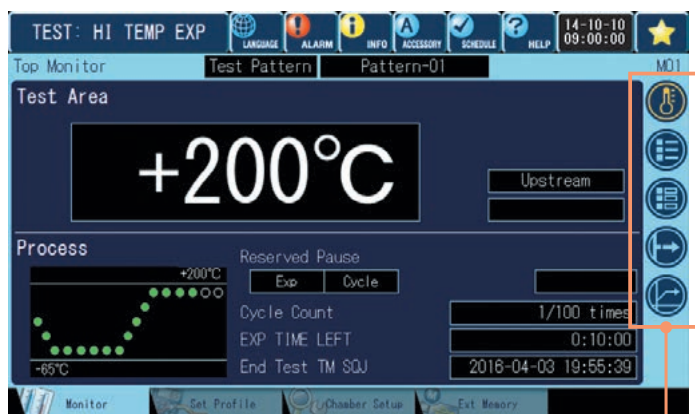

Slide label

Touching an icon displays the menu label.



Tabbed interface

High resolution 7-inch LCD. Tabs at the bottom make for quick and easy flipping between screens. Touching an icon displays the menu label which, touched, makes flipping between screens easier.

Multilingual display

Use the language icon at the top of the display to change the display language from Japanese to English, Simplified Chinese, Traditional Chinese or Korean on any screen.

Quick access button

For added convenience, the star (★) icon can have quick access functionality assigned, such as for jumping to a certain screen or directly launching a saved test pattern.


Test data records

Temperature settings and measurements can be stored in the internal memory and exported with the use of USB flash drives. This enables them to be displayed as graphs on web browsers and stored for back-up purposes.

Test data can also be recorded in real time to a USB flash drive.

* USB flash drives not included.

Program copy and computer editing

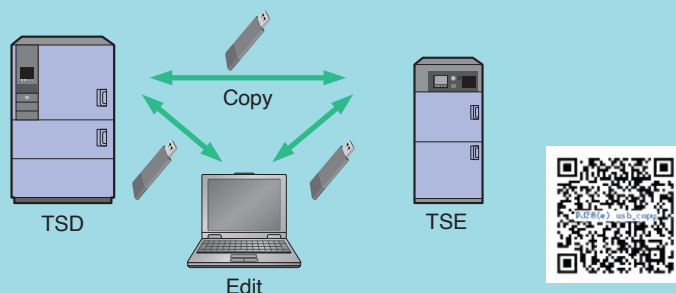

* Some items may not be copied between different models and chambers with different options.



USB memory port

Register up to 40 test patterns

Download edit programs via online

The Pattern Manager Lite software installed on your PC, edit programs according to your testing needs, and upload them with a USB.

The Pattern Manager Lite software allows you to edit programs for your chamber, view and edit data as graph, etc. The software can be downloaded from the Test Navi website.

Network

- * Requires an intranet
- * Supported browser: Internet Explorer 11

Remote monitor and control (Ethernet connection)

The chamber comes with an ESPEC original web application. Connecting to the chamber Ethernet port (LAN's port) makes it possible to control chamber monitoring, pattern setting, operation start/stop, and other operations from a computer web browser. Installation of special software is not required. All you need is a standard computer web browser to connect with the chamber.

Login privileges

Screen Privileges	Chamber monitor	Pattern setting	Run/ Stop	Configuration
Administrator	✓	✓	✓	✓
Operator	✓	✓	✓	
User	✓			

Edit test patterns on a web browser

Saved test programs can be edited on a web browser. Test programs can also be downloaded to your PC.

E-mail alert

Alerts such as for a test ending, for maintenance, and errors are e-mailed to multiple recipients.

Wireless LAN connection



Watch the videos


► Remote ON/OFF Operation




► Connecting Easily with Ethernet (LAN)



Email alert

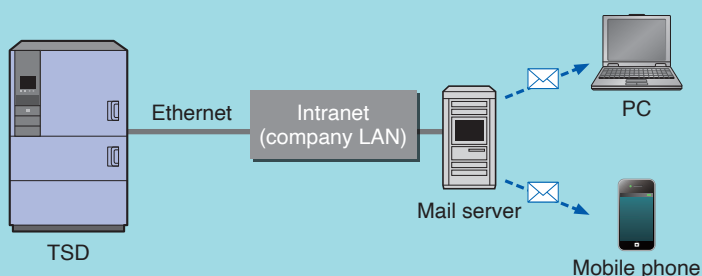

ESPEC OnlineCore (Sold separately)
Central control system recommended for multiple environmental test chambers installations

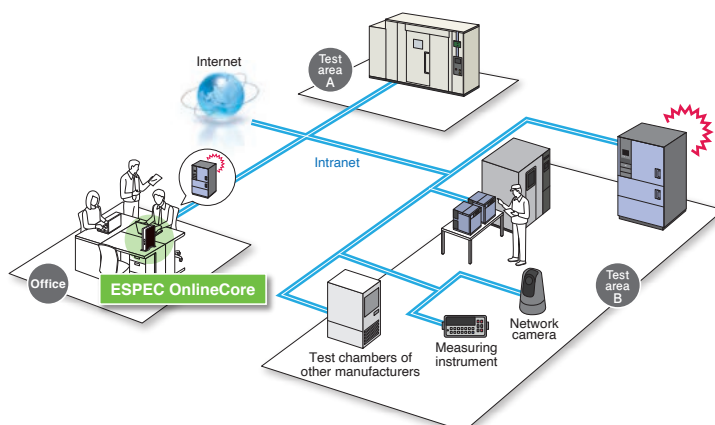

*Please contact ESPEC for more information, about which products can be connected.

Model			TSD-101-W						
			Water-cooled						
System			2-zone transition by vertical transfer of specimens						
Performance ^{*1}	Test area	Hot exposure range	+ 60°C to + 205°C						
		Cold exposure range	− 77°C to 0°C						
		Temp. fluctuation ^{*2}	± 1.0°C						
	Hot chamber	Pre-heat upper limit	+ 205°C						
		Heat-up time ^{*3}	Within 90 min from ambient temp. to + 200°C (Setting: + 205°C)						
	Cold chamber	Pre-cool lower limit	− 77°C						
		Pull-down time ^{*3}	Within 90 min from ambient temp. to − 77°C (Setting: − 77°C)						
	Temp. recovery performance (2-zone)	Recovery conditions	• Hot exposure: + 150°C (setting: + 155°C 30 min) • Cold exposure: − 65°C (setting: − 68°C 30 min) • Sensor position: downstream • Specimen: Plastic molded ICs, 10kg						
			Temp. recovery time	Specimen temp. within 15 min					
	Transfer time between hot & cold chambers			Within 10 seconds					
Ambient recovery	Recovery conditions	• Hot exposure: + 150°C to max. + 55°C • Ambient temp.: + 23°C • Specimen: Plastic molded ICs, 10 kg							
		Ambient temp. recovery time	Within 90 min						
Test area			Shelf brackets on 2 levels (up to 4 baskets can be installed)						
Refrigeration unit	System	Mechanical cascade refrigeration system							
	Compressor	3.73kW(5HP) scroll-type × 2							
	Refrigerant	R-404A [R-449A is available on request] , R-23							
Cooler			Plate fin cooler and cold accumulator						
Elevating unit			Power slider (250W)						
Fittings			USB memory port, Ethernet port (LAN port), specimen power supply control terminal, time signal output terminal (× 2), specimen temperature input terminal (× 2), cable port ID ϕ 100mm on right side (left side available as option), *Power cables not included.						
Inside dimensions			W710×H345×D410 mm						
Test area capacity			100 L						
Load capacity of test area ^{*4}			30 kg						
Outside dimensions ^{*5}			W1100×H1885×D1965 mm						
Weight			Approx. 1100 kg						
Utility requirements	Ambient temp. range		+ 5°C to + 40°C						
	Power supply (Voltage fluctuation: rating ± 10%)		200V AC 3 ϕ 3W 50/60Hz	208V AC 3 ϕ 3W 60Hz ^{*6}	220V AC 3 ϕ 3W 60Hz	380V AC 3 ϕ 4W 50Hz	400/415V AC 3 ϕ 4W 50Hz ^{*7}		
	Maximum load current		64 A	62 A	58 A	34 A	32 A		
	Cooling water supply pressure ^{*8}		0.2 Mpa to 0.5 Mpa (2 kg/ cm²G to 5 kg/ cm²G)						
	Cooling water supply rate ^{*9}		2050L/ h (at reference water temp. + 25°C), 3400L/ h (at reference water temp. + 32°C)						
	Piping connection size		Carbon steel pipe, ID 32 mm						
	Cooling water temp. range		+ 5°C to + 38°C						
Noise level ^{*10}			Max. 65 dB						
Exhaust heat rate			12600 kJ/h (3000 kcal/h)						
Exhaust air volume			250 m³/h						

^{*1} Under the conditions of a + 23°C ambient temperature, cooling water temperature + 25°C, rated voltage, and no specimen inside the test area.

^{*2} The performance values are based on IEC 60068-3-5:2001,

^{*3} When each chamber is operated independently

^{*4} When using the test area floor or heavy-duty shelves (option)

^{*5} Excluding protrusions

^{*6} This model complies with the requirements of the National Electric Code (NFPA 70) for the United States of America (NEC spec.)

^{*7} This model complies with the requirements of the European Community Directives (CE spec.)

^{*8} A pressure regulator valve is required if the pressure exceeds 0.5MPa (5kg/cm²G)

^{*9} Rate depends on the cleanliness of the heat exchanger

^{*10} Measurements are to be taken in an anechoic room at a height of 1.2m from the floor, and a distance of 1m from the front panel (ISO 1996-1: 2003.A-weighted sound pressure level)

SAFETY DEVICES

TSD-101-W

- Leakage breaker (200, 220V AC)
- Circuit breaker (208, 380, 400/415V AC)
- Electrical compartment door switch
- Hot chamber overheat protection switch
- Cold chamber overheat protection switch
- Hot chamber overheat protector
(Built into temperature controller)
- Cold chamber overheat/ overcool protectors
(Built into temperature controller)
- Test area overheat/ overcool protectors
(Built into temperature controller)
- Test area overheat/ overcool protectors
- Circuit breaker
- Refrigerator high/ low pressure switch
- Compressor built-in protector
- Temperature switch for compressor
- Water suspension relay
- Temperature switch for air circulator
- Air circulator thermal relay
- Motor inverter
- Motor reverse prevention relay
- Hot chamber door switch
- Cold chamber door switch
- Door lock mechanisms
- Cartridge fuse
- Specimen power supply control terminal
- Cooling tower interlock terminal

ACCESSORIES

TSD-101-W

- Specimen basket
(18-8 Cr-Ni stainless steel: 5 mesh metal basket)
W700×H40×D410 mm/ load capacity 5kg 2



- Shelf brackets 2 sets
- Cartridge fuse (3A, 5A, 7A, 10A, 15A) 4
- Cable port rubber plug 2
- Perforated cable port cap 1
- Wire fisher (specimen wiring tool) 1
- Thermocouple 2
- Specimen temperature input connector 2
- 3-pole socket (208V AC spec. only) 3
- Nipple R1 1/4 in. (32 A) 1
- Strainer R1 1/4 in. (32 A) 1
- Strainer element R1 1/4 in. (32 A) 1
- Breaker handle cover (except 208V AC) 1
- Operation manual 1

SIZE VARIATION

70L/300L

Model		TSD-71-A	TSD-301-W
		Air-cooled	Water-cooled
Hot exposure range		+ 60°C to + 205°C	+ 65°C to + 200°C
Cold exposure range		− 77°C to 0°C	− 65°C to 0°C
Temp. recovery performance (2-zone)	Recovery conditions	<ul style="list-style-type: none"> • Hot exposure: + 150°C (setting: + 155°C 30 min) • Cold exposure: − 65°C (setting: − 68°C 30 min) • Sensor position: downstream • Specimen: Plastic molded ICs, 5kg 	<ul style="list-style-type: none"> • Hot exposure: + 150°C (30 min) • Cold exposure: − 65°C (30 min) • Sensor position: downstream • Specimen: Plastic molded ICs, 20kg
	Temp. recovery time	Specimen temp. within 15 min	Specimen temp. within 30 min
Inside dimensions		W560×H345×D370 mm	W650×H655×D650 mm

Model			TSE-12-A			
			Air-cooled			
System			2-zone transition by vertical transfer of specimens			
Performance ^{*1}	Test area	Hot exposure range	+ 60℃ to + 200℃			
		Cold exposure range	− 65℃ to 0℃			
		Temperature fluctuation ^{*2}	± 0.5℃			
	Hot chamber	Pre-heat upper limit	+ 205℃			
		Heat-up time ^{*3}	Within 30 min. from ambient temp. to + 200℃ (Setting: + 205℃)			
	Clod chamber	Pre-cool lower limit	− 82℃			
		Pull-down time ^{*3}	Within 90 min. from ambient temp. to − 80℃ (Setting: − 82℃)			
	Temp. recovery performance (2-zone)	Recovery conditions	· Hot exposure: + 150℃, 30 min · Cold exposure: − 65℃, 30 min · Sensor position: Upstream · Specimen: Plastic molded ICs 2 kg			
		Temp. recovery time	Within 5 min.			
Transfer time between hot & cold chambers			Within 10 seconds			
Construction	Test area		Shelf brackets on 2 levels of fixed location			
	Heater		Stripped wire heater			
	Refrigeration unit	System	Mechanical cascade refrigeration system			
		Compressor	Rotary 1.5 kW × 2			
		Refrigerant	R-404A (R-449A is available on request) , R-508A			
	Cooler		Plate fin cooler and cold accumulator			
Elevating unit		Linear motor (55W)				
Fittings			USB memory port, Ethernet port (LAN port), specimen power supply control terminal, time signal output terminal (2), cable port ID ϕ 50mm on right side, casters with leveling feet (4), power cable (approx. 2.5m)			
Test area capacity			W320 × H148 × D230mm			
Inner volume of test area			10.9 L			
Load capacity of test area			8 kg			
Outside dimensions ^{*4}			W680 × H1745 × D1050mm			
Weight			Approx. 400kg			
Utility requirements	Ambient temp. range		0℃ to + 40℃			
	Power supply (Voltage fluctuation: rating ± 10%)		200V AC 3 ϕ 3W 50/60Hz	220V AC 3 ϕ 3W 60Hz	380V AC 3 ϕ 4W 50Hz	400/415V AC 3 ϕ 4W 50Hz ^{*5}
	Maximum load current		26A	25A	17A	17A
Noise level ^{*6}			Max.60dB			
Exhaust heat rate ^{*7}			17,585kJ/h (4200 kcal/h)			

^{*1} The performance values are under the conditions of a +23°C ambient temperature, relative humidity of 65%rh, rated voltage, and no specimen. Heat up time and pull down time are those of single-unit operation of each chamber.

^{*2} The performance values are based on IEC60068-3-5:2001.

^{*3} Temperature heat-up/pull-down time account for performance of each temperature chamber.

^{*4} Excluding protrusions.

^{*5} Compliance with CE Marking.

^{*6} At 1m from front of chamber, 1.2m from floor. (ISO 1996-1:2003 A-weighted sound pressure level) depending on environment

^{*7} At ambient temperature +23°C.

SAFETY DEVICES

TSE-12-A

- Leakage breaker (200, 220V AC)
- Circuit breaker (380, 400 / 415V AC)
- Electrical compartment door switch
- Hot chamber overheat protection switch
- Cold chamber overheat protection switch
- Hot chamber overheat protector
(Built into temperature controller)
- Cold chamber overheat / overcool protectors
(Built into temperature controller)
- Test area overheat and overcool protectors
(Built into temperature controller)
- Test area overheat / overcool protectors
- Refrigerator high pressure switch
- Thermal relay for compressor
- Temperature switch for compressor
- Temperature switch for air circulator
- Thermal relay for air circulator
- Motor inverter
- Motor reverse prevention relay
- Hot chamber door switch
- Cold chamber door switch
- Test area hold
- Door lock mechanisms
- Fuse
- Specimen power supply control terminal

ACCESSORIES


TSE-12-A

- Specimen basket
(18-8 Cr-Ni stainless steel, 5 mesh metal basket)
W320×H35×D230mm /load capacity: 2kg 2



- Cartridge fuse
3A, 5A (200/220V AC) 1each
3A, 5A, 7A (380/400/415V AC) 1each
- Cable port rubber plug 2
- Wire fisher (specimen wiring tool) 1
- Breaker handle stopper (200/220V AC only)
- Operation manual 1

● Fittings location

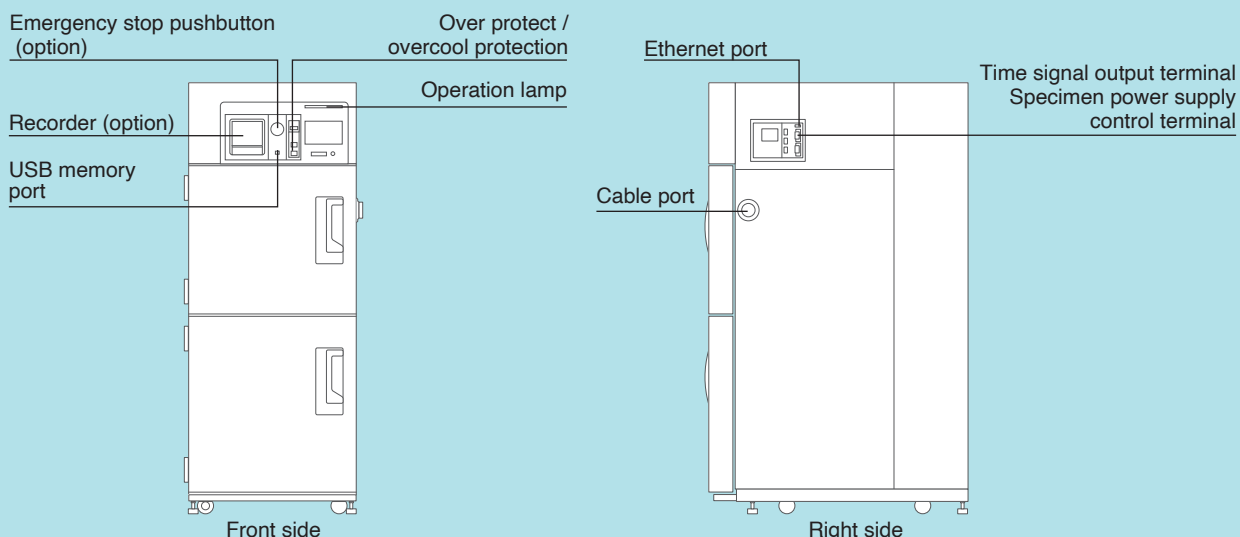

Safety precautions

- Do not use specimens which are explosive or inflammable, or which contain such substances. To do so could be hazardous, as this may lead to fire or explosion.
- Do not place corrosive materials in the chamber. If corrosive substances or humidifying water is used, the life of the unit may be significantly shortened.
- Do not place life forms or substances that exceed allowable heat generation.
- Be sure to read the operation manual before operation.

OPTIONS

TSD-101-W / TSE-12-A

Power cable

- 5 m
- 10 m

〈TSD〉

* Not applicable for optional 208, 380 and 400/415V AC power supply specification.

* If this option is not specified, the chamber does not come with a power cable.

Viewing window

TSD

Used for observation of the specimens inside the chamber.

Dimensions: W190 × H340 mm

Chamber lamp: Halogen lamp (× 1)



Specimen basket/ shelf brackets

Equivalent to standard accessory.
Material: Stainless steel (5 mesh)

〈TSD〉

- Basket
- Shelf brackets

〈TSE〉

- Basket

Heavy-duty shelf

TSD

Used to hold heavy specimen exceeding the load capacity of the standard specimen basket.

Load capacity: 15 kg

* Equally distributed load, not included shelf brackets and specimen baskets.

Additional cable port

TSD

Provided in addition to the standard cable port. (right side)

Location: Left side of the main unit

Internal diameter: 100 mm

Cable port rubber plug

Prevents air leakage from the cable port.

Interface

- RS-485C
- RS-232C
- GPIB

Communication cables

- RS-485C 5m/10m/30m
- GPIB 2m/4m

Temperature recorder (digital)

— 100 to + 220°C /100 mm

- RK-61: 1 pen
- RK-63: 3 pens
- RK-64: 6 dots



Paperless recorder

Records temperature of each section such as the temperature inside the chamber.

Display: 5.7inch color touch panel

Number of inputs (Initial setting):

- 1 (5 more channels can be turned ON)
Data saving cycle: 1 sec
- 3 (3 more channels can be turned ON)
Data saving cycle: 1 sec
- 3 (3 more channels can be turned ON)
Data saving cycle: 5 sec
- 5 (1 more channels can be turned ON)
Data saving cycle: 1 sec
- 5 (1 more channels can be turned ON)
Data saving cycle: 5 sec
- 6 Data saving cycle: 1 sec
- 6 Data saving cycle: 5 sec

Temperature range: — 100 to + 220°C

Internal memory: 8MB

External memory media:

CF memory card (256 MB)

External memory function: USB port

Language support: ENG/ JPN

* Select either built-in or portable type. (TSD)



Recorder wiring

Preparation of a power cable, temperature sensor, and a grounding wire for additional installation in the future.

Recorder terminal

Used to output the temperature within test area, hot chamber, cold chamber.

Thermocouple

Attached to specimens to measure specimen temperature.

〈TSD〉

Thermocouple type T without ball
(Copper/ Copper-Nickel)

〈TSE〉

T JIS C1602 with ball attached

- 2 m
- 4 m
- 6 m

STT 3-point expansion

TSD

Additional 3 points of measuring the specimens' temperatures used for Specimen Temperature Trigger function.
(2 points are equipped as standard.)

Exposure signal output

TSD

A signal is output via a contact switch when test area temperature is within the user-selected range. This signal can be used to control peripheral instruments, like applying a voltage to specimens only during hot exposure, or monitoring test operation from a remote point.

Total cycle counter

Indicates cycle counts.

Display range: 1-99999999

(with resetting function)



Additional overhear protector

Additional preventive measures can be taken for excessive temperature rise in the chamber, in addition to the standard equipped double overhear protector.

Emergency stop pushbutton

Stops the chamber immediately.



With cover



With guard



Auxiliary cooling injector (LCO₂)

Used to reduce the temperature recovery time of low temperature exposure by injecting liquefied carbon dioxide at beginning of exposure.


Auxiliary cooling injector (LN₂)

Used to reduce the temperature recovery time of low temperature exposure by injecting liquefied nitrogen at beginning of exposure.



External alarm terminal

If the safety device of the chamber is activated, the external alarm terminal will notify it to a remote point.



TSD

Anchoring fixtures

Used to bolt the chamber to the floor.

Chamber dew tray

Prevents water leakage from the chamber onto the floor.

* The use of casters is recommended to facilitate operation. (TSD)

* To prevent damage in the event of water leakage, other preventive measures are also available.

Casters

TSD

Installed for mobility.

Casters: 6

levelling-feet: 4



Operation manual

- CD
- Booklet

Reports & certificates

- Testing and inspection report
- Test data
- Calibration report
- Calibration certificate
- Traceability system chart
- Traceability certificate

ESPEC CORP. <https://www.espec.co.jp/english>

Head Office

3-5-6, Tenjinbashi, Kita-ku, Osaka 530-8550, Japan
Tel: 81-6-6358-4741 Fax: 81-6-6358-5500

ESPEC NORTH AMERICA, INC.

Tel: 1-616-896-6100 Fax: 1-616-896-6150

ESPEC EUROPE GmbH

Tel: 49-211-361850-0

ESPEC ENVIRONMENTAL CHAMBERS

SALES AND ENGINEERING LTD. STI. (Turkey)

Tel: 90-212-438-1841 Fax: 90-212-438-1871

ESPEC ENVIRONMENTAL EQUIPMENT (SHANGHAI) CO., LTD.

Head Office

Tel: 86-21-51036677 Fax: 86-21-63372237

BEIJING Branch

Tel: 86-10-64627025 Fax: 86-10-64627036

GUANGZHOU Branch

Tel: 86-20-83317826 Fax: 86-20-83317825

SHENZHEN Branch

Tel: 86-755-83674422 Fax: 86-755-83674228

SUZHOU Branch

Tel: 86-512-68028890 Fax: 86-512-68028860

TIANJIN Branch

Tel: 86-22-26210366 Fax: 86-22-26282186

XI'AN Branch

Tel: 86-29-88312908 Fax: 86-29-88455957

CHENGDU Branch

Tel: 86-28-88457756 Fax: 86-28-88474456

WUXI Branch

Tel: 86-510-82735036 Fax: 86-510-82735039

ESPEC TEST TECHNOLOGY (SHANGHAI) CO., LTD.

Tel: 86-21-68798008 Fax: 86-21-68798088

ESPEC ENGINEERING (THAILAND) CO., LTD.

Tel: 66-3-810-9353 Fax: 66-3-810-9356

ESPEC ENGINEERING VIETNAM CO., LTD.

Tel: 84-24-22208811 Fax: 84-24-22208822

ISO 9001 (JIS Q 9001)

Quality Management System Assessed and Registered

ESPEC CORP. has been assessed by and registered in the Quality Management System based on the International Standard ISO 9001:2015 (JIS Q 9001:2015) through the JSA Solutions Co.,Ltd.

* The organization of these certificates is
ESPEC CORP. Japan.



ISO 27001 (JIS Q 27001)

Quality Management System Assessed and Registered

* The organization of these certificates is
ESPEC CORP. Japan.



ISO 14001 (JIS Q 14001)

Environmental Management System Assessed and Registered

* The organization of these certificates is
ESPEC Group Japan.

